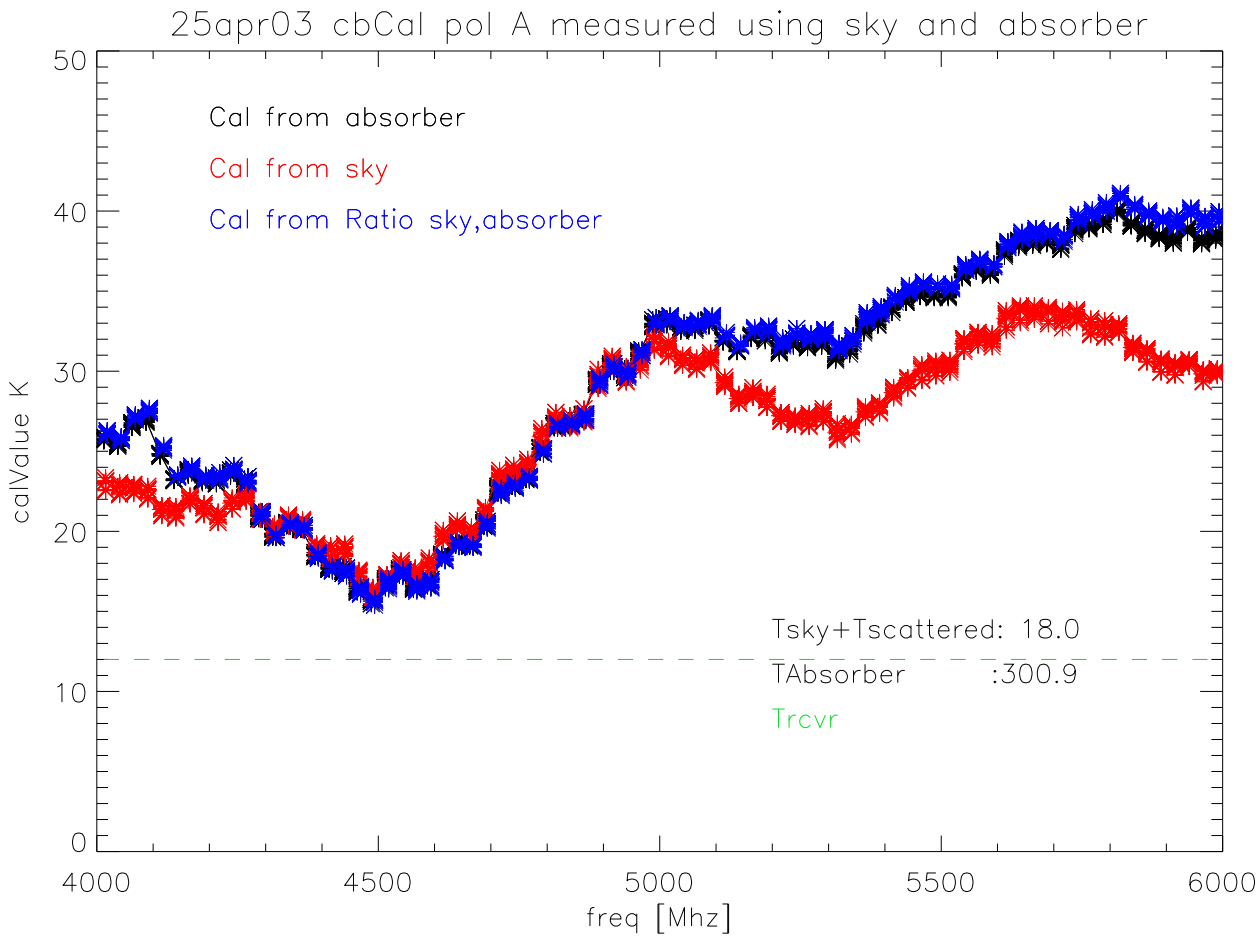
25apr03 cbCal pol A measured using sky and absorber
Cal from absorber
Cal from sky
Cal from Ratio sky,absorber
Tsky+Tscattered: 18.0
TAbsorber :300.9
Trcvr
calValue K
freq [Mhz]
0
10
20
30
40
50
4000
4500
5000
5500
6000

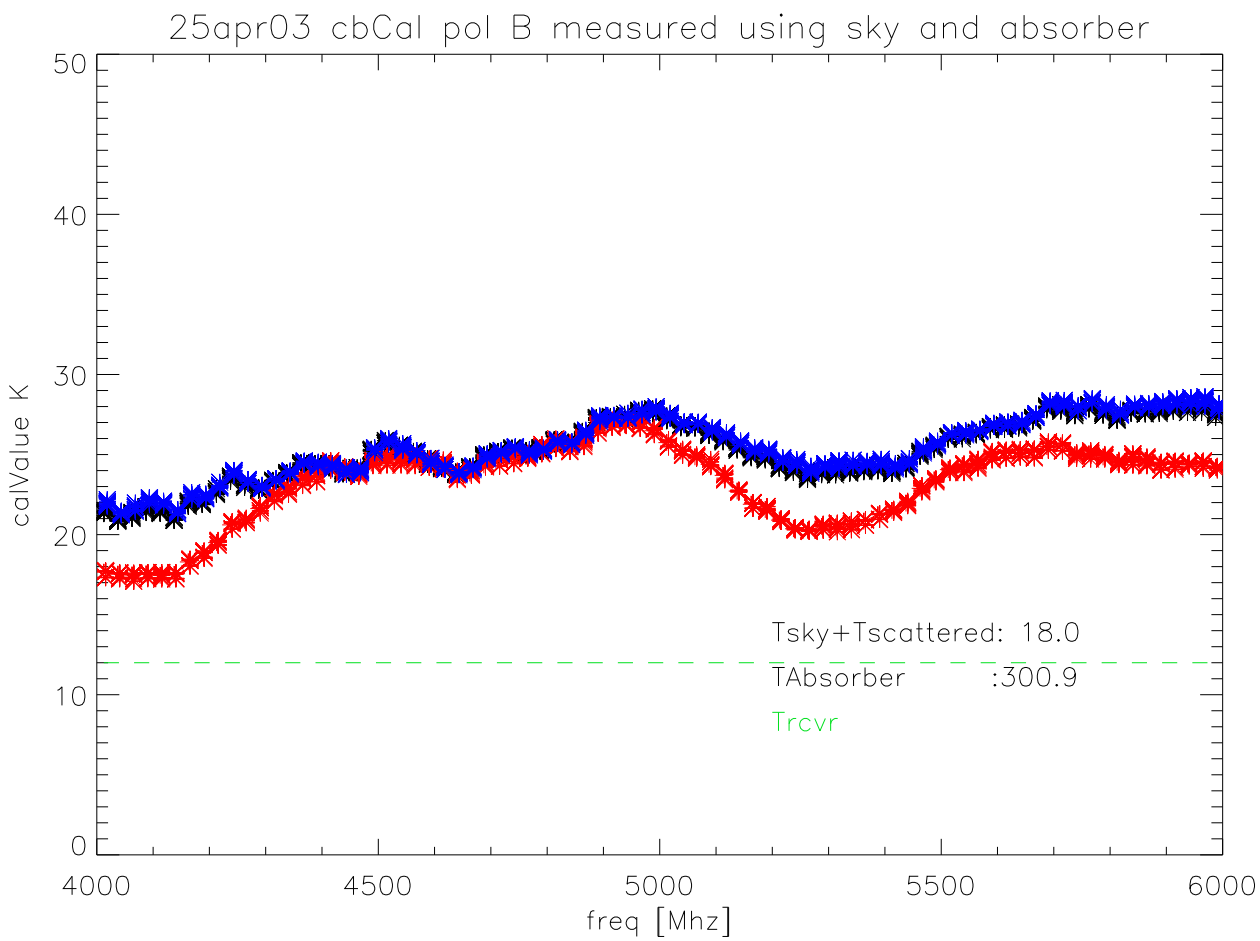
25apr03 cbCal pol B measured using sky and absorber
Tsky+Tscattered: 18.0
TAbsorber :300.9
Trcvr
calValue K
freq [Mhz]
0
10
20
30
40
50
4000
4500
5000
5500
6000

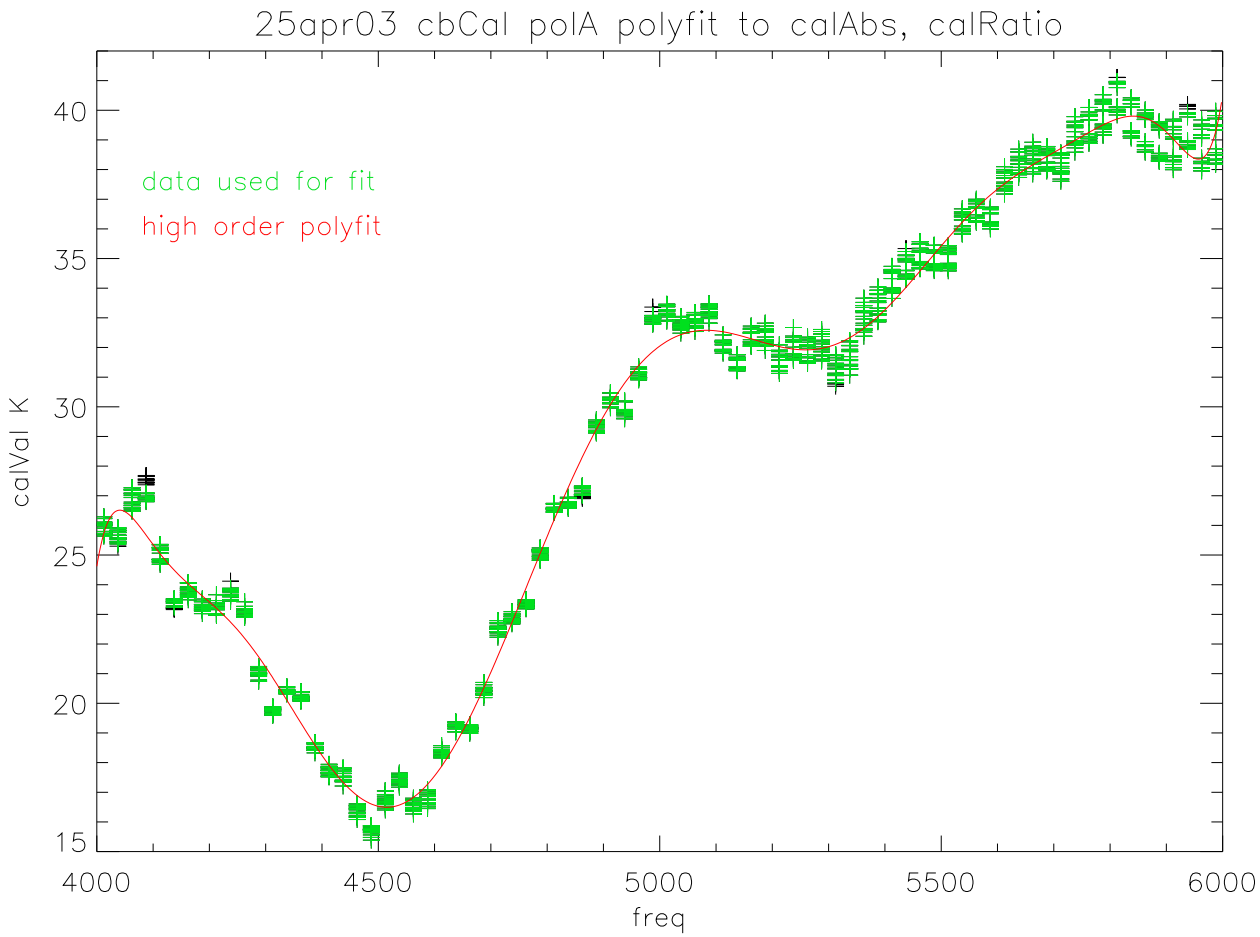
25apr03 cbCal polA polyfit to calAbs, calRatio
data used for fit
high order polyfit
calVal K
freq
40
35
30
25
20
15
4000
4500
5000
5500
6000

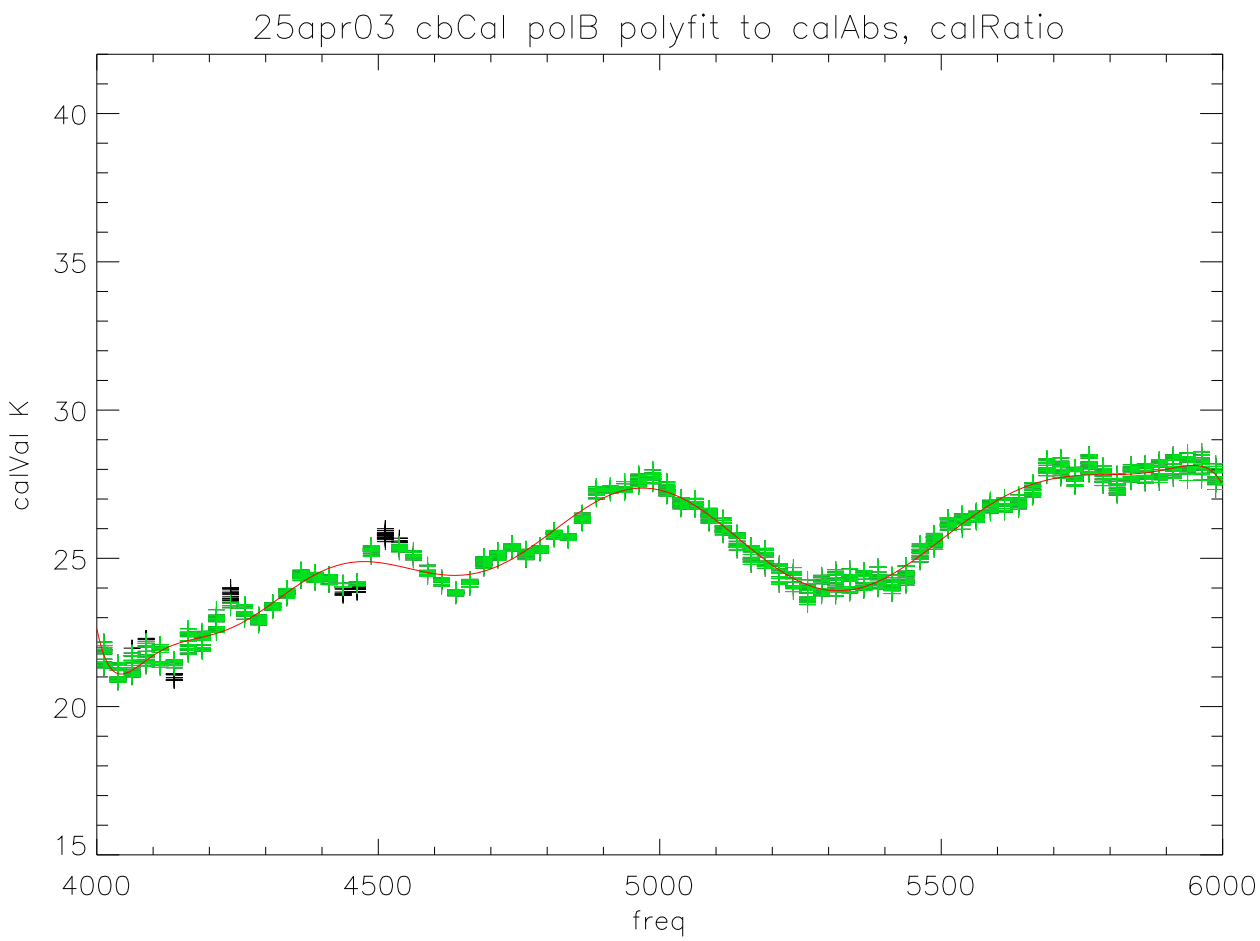
25apr03 cbCal polB polyfit to calAbs, calRatio
calVal K
freq
40
35
30
25
20
15
4000
4500
5000
5500
6000

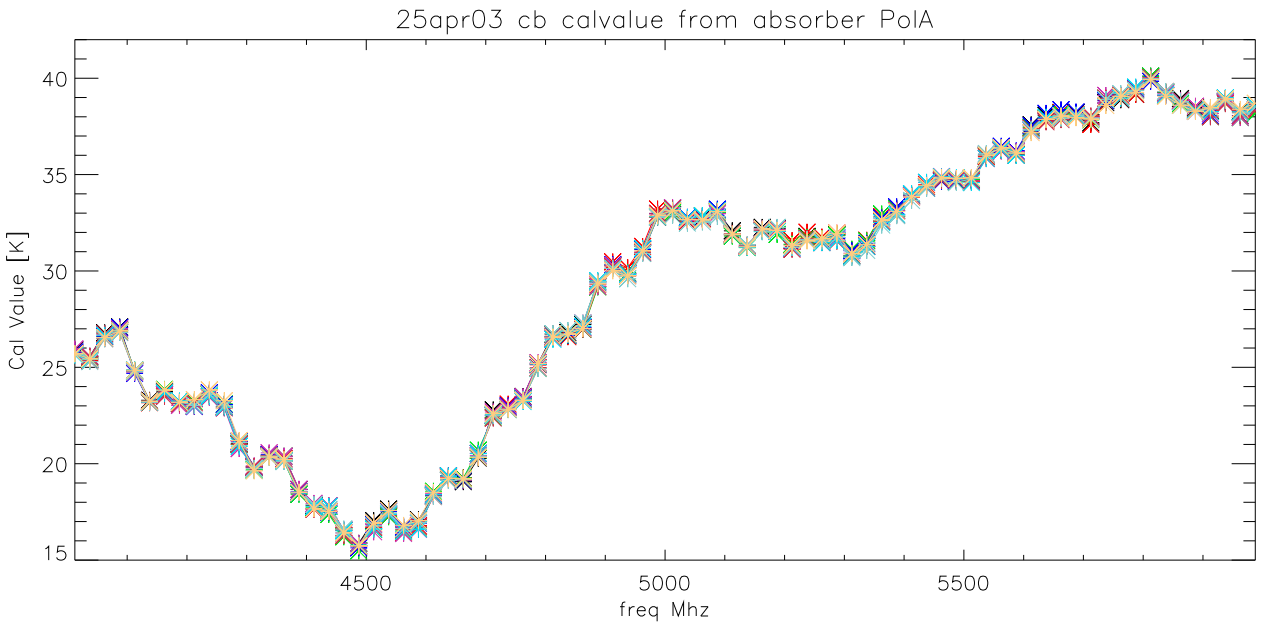
25apr03 cb calvalue from absorber PolA
Cal Value [K]
40
35
30
25
20
15
4500
5000
5500
freq Mhz

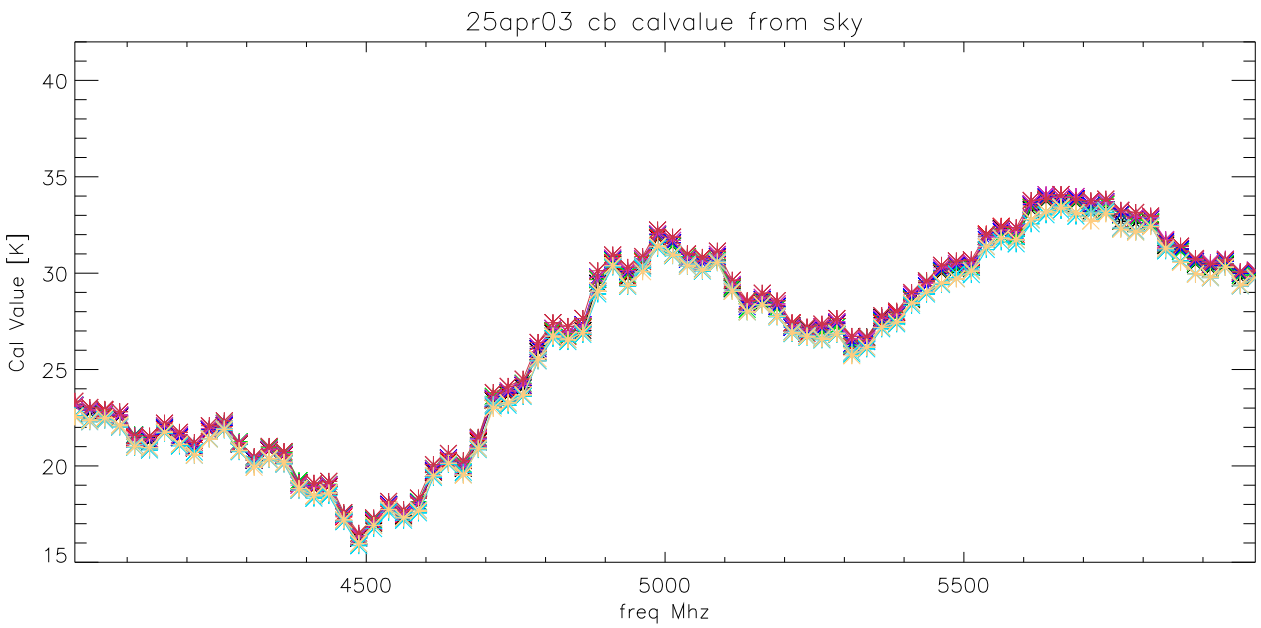
25apr03 cb calvalue from sky
Cal Value [K]
40
35
30
25
20
15
4500
5000
5500
freq Mhz

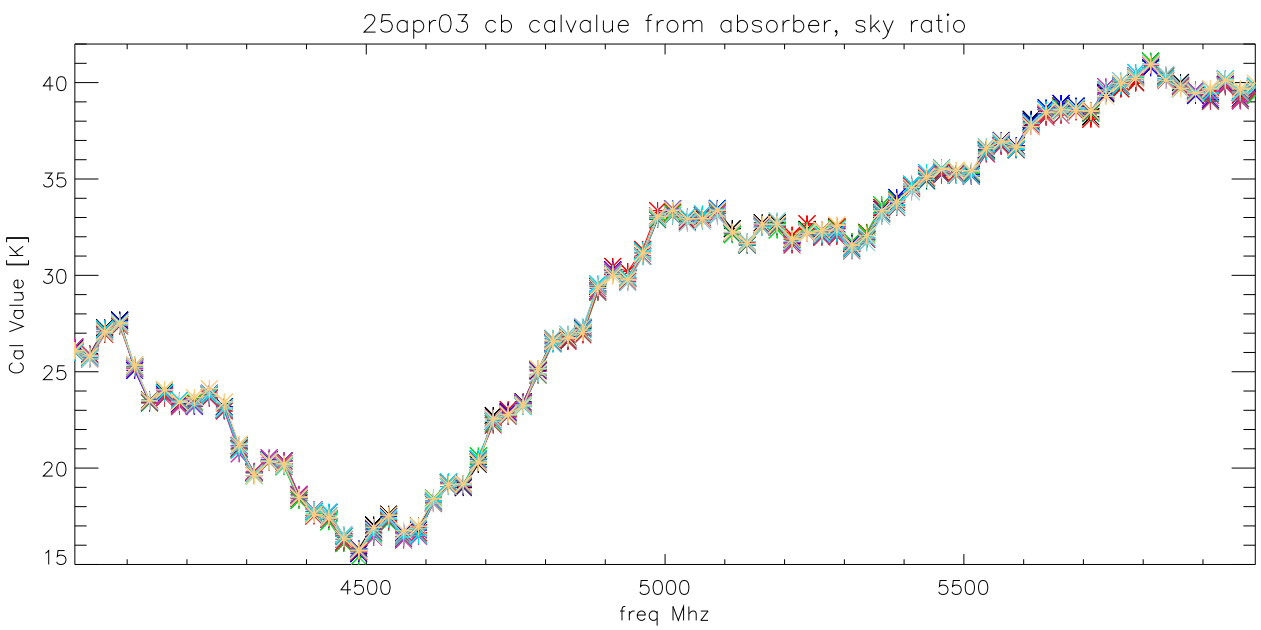
25apr03 cb calvalue from absorber, sky ratio
Cal Value [K]
40
35
30
25
20
15
4500
5000
5500
freq Mhz

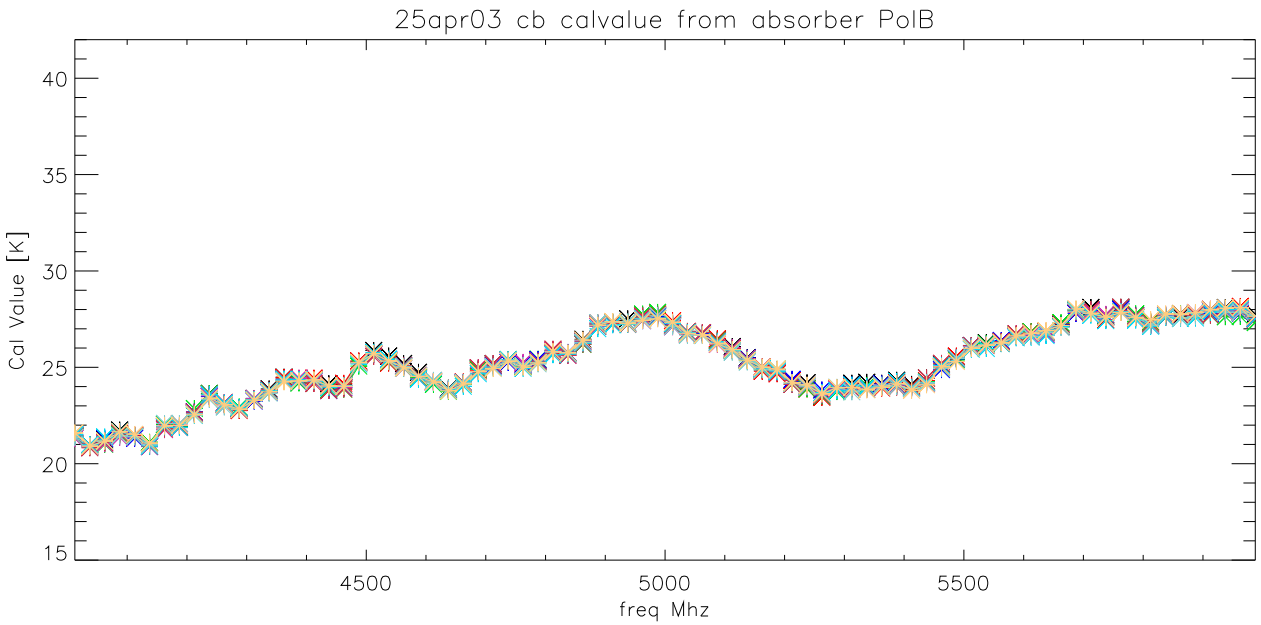
25apr03 cb calvalue from absorber PolB
Cal Value [K]
40
35
30
25
20
15
4500
5000
5500
freq Mhz

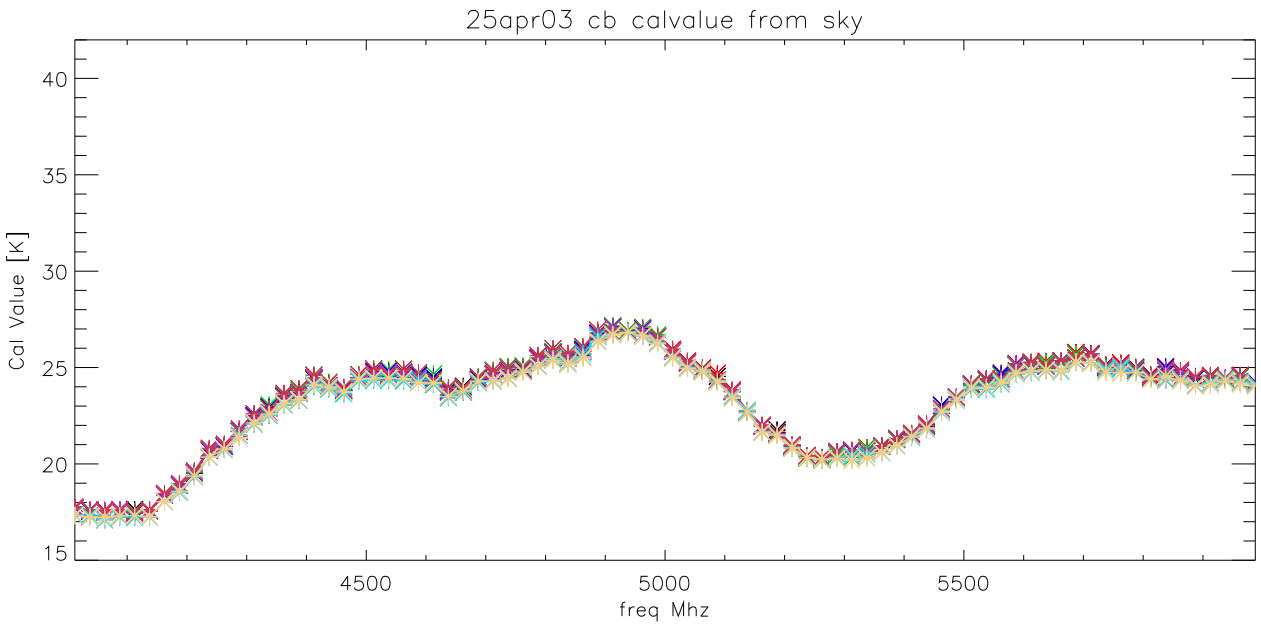
25apr03 cb calvalue from sky
Cal Value [K]
40
35
30
25
20
15
4500
5000
5500
freq Mhz

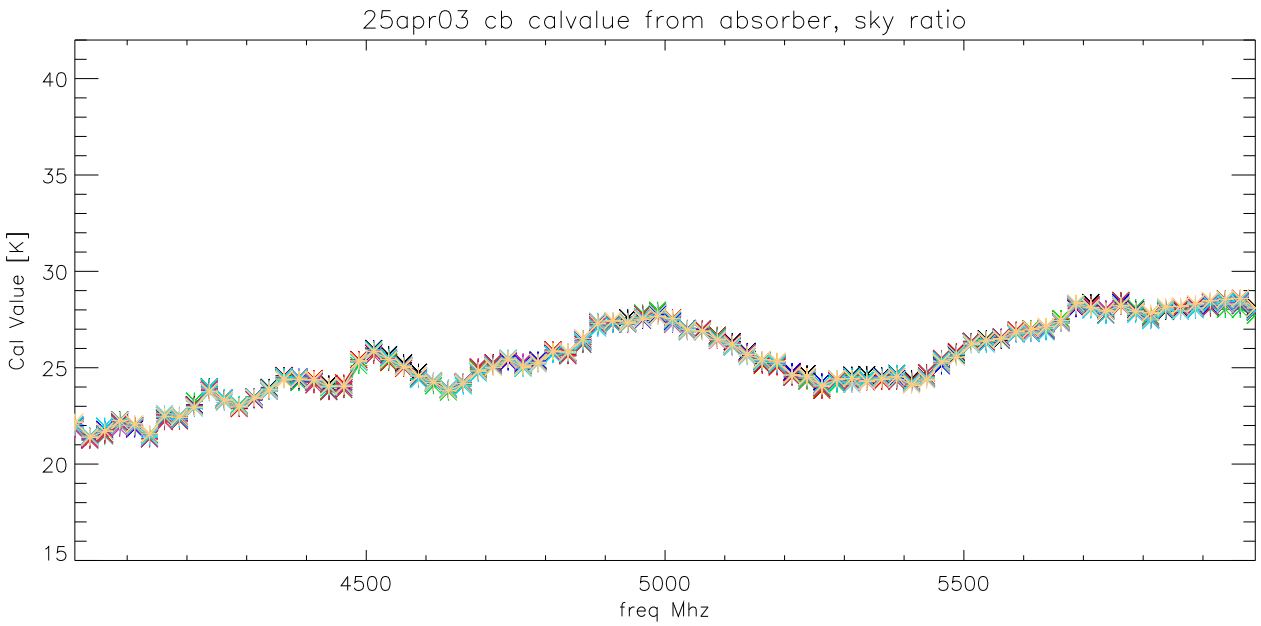
25apr03 cb calvalue from absorber, sky ratio
Cal Value [K]
40
35
30
25
20
15
4500
5000
5500
freq Mhz